

Fig. 1

a (Baseline)

b (15 sec p.i.)

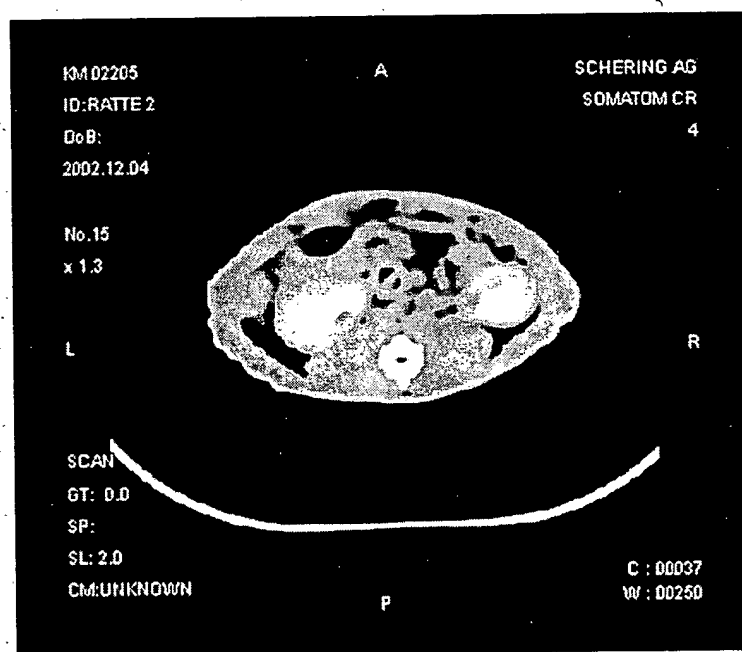


Fig. 2 CT Image of a Rat 15 Minutes after I.V. Injection of IB

BEST AVAILABLE COPY

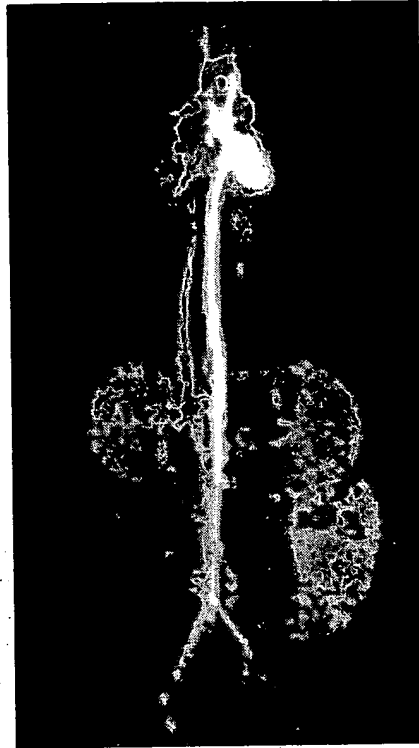


Fig. 3 MRA 7.5 Seconds After I.V. Injection of IB in Rats

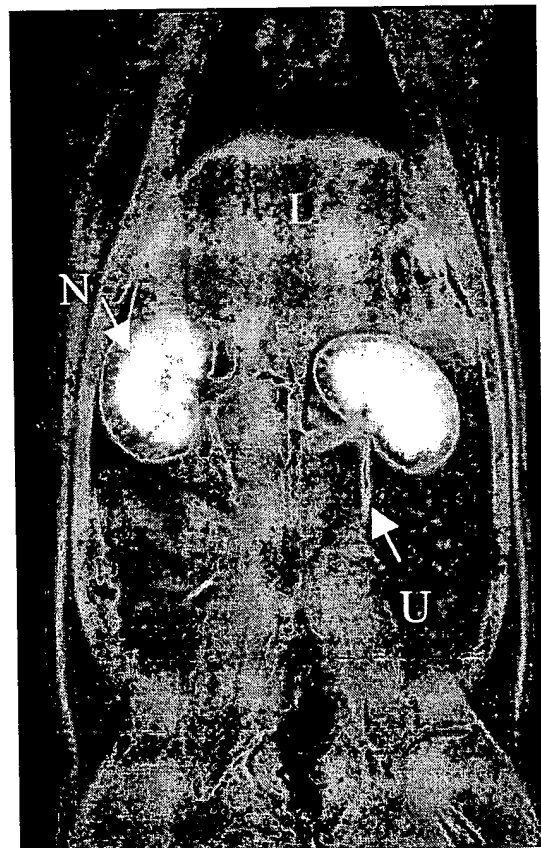
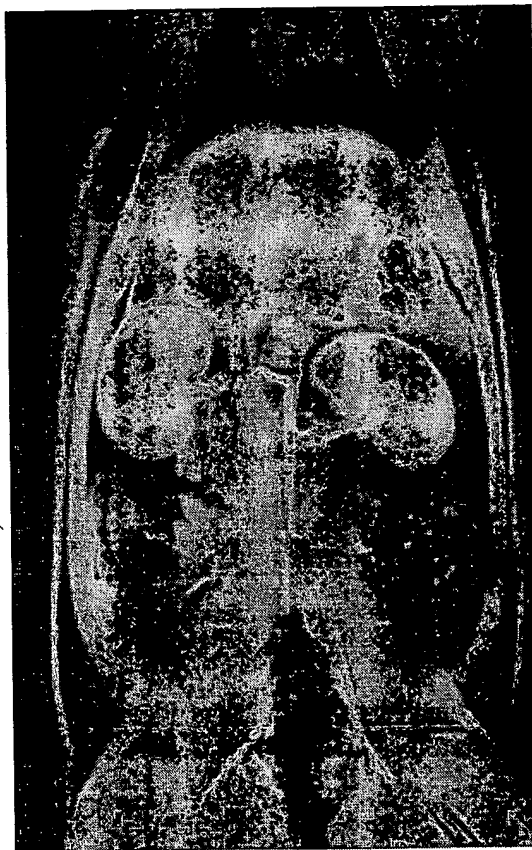


Fig. 4

a (Baseline)

b (15 min p.i.)

BEST AVAILABLE COPY

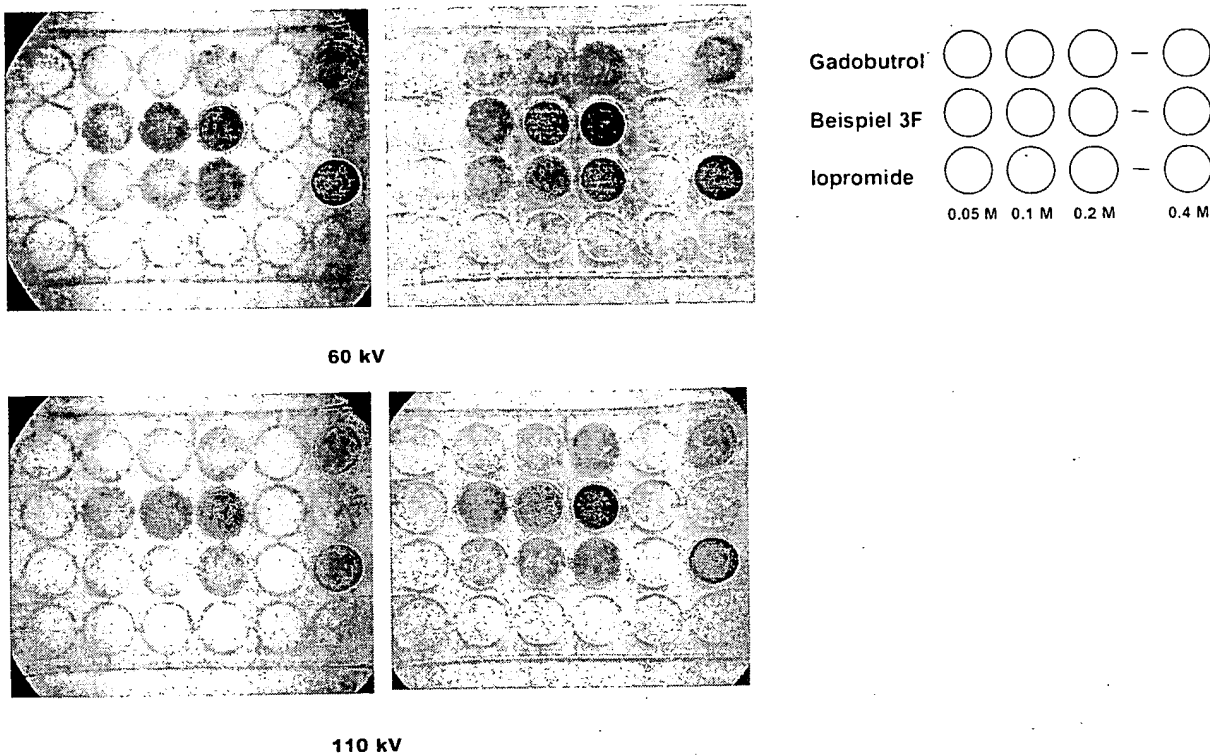


Figure 5: Comparison of X-ray Absorption of Example 3F, Gadobutrol and Iopromide X-ray images of the phantom at 60 and 110 kV anode voltage are recorded with the C-arm device stenoscope D6 (General Electric).

[Key to Fig. 5:] Beispiel 3F = Example 3F

BEST AVAILABLE COPY

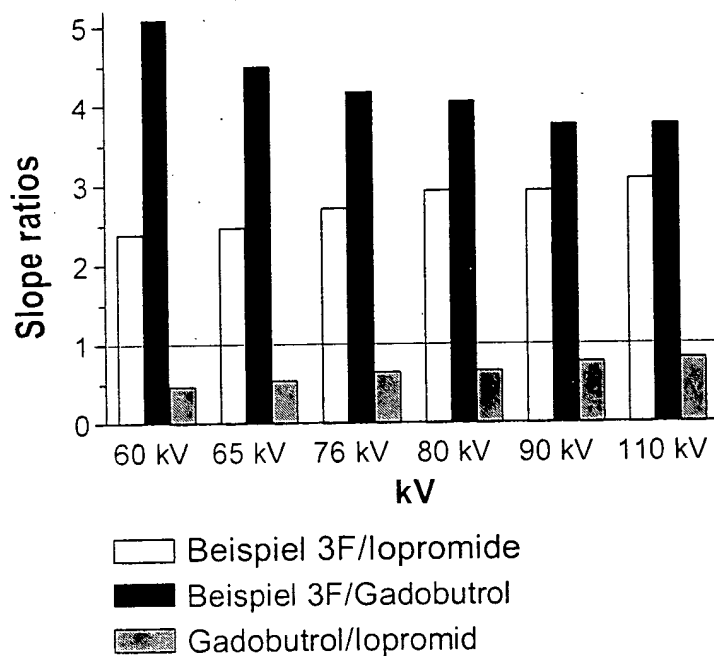


Figure 6: Relative X-ray Absorption of Example 3F in Comparison with Gadobutrol and Iopromide at Various Anode Voltages of X-ray Tubes (Stenoscope D6, General Electric).
[Key to Fig. 6:] Beispiel = Example, Iopromid = Iopromide